

# access

STERILE R

## GO-GLIDER


Variable taper

**Pre-enlarger**



Endodontic sequence in NiTi  
up to **50% cheaper**

**Try**



**GO-GLIDER**

SATISFIED or MONEY BACK\*

STANDARD CASES

With heat treatment




**FLEXIBILITY**




**FOAM GUIDE TIPS**

WITH **GO-GLIDER**


**SIMPLIFIED  
PREPARATION WITH  
1 SINGLE INSTRUMENT!**

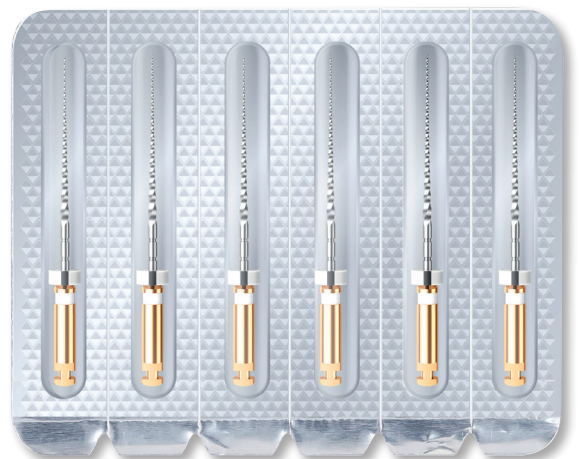


GO-GLIDER




Flexibility



Cutting power



Resistance



Single use

FLEXIBILITY AND ENDURANCE

FOR TREATMENT


x6



GO-GLIDER	LENGTH		
	21 mm	25 mm	31 mm
2% – ISO 016	3166663	3166664	3166665

ALL THE PREPARATION  
JUST WITH 1 FILE !

STANDARD CASES

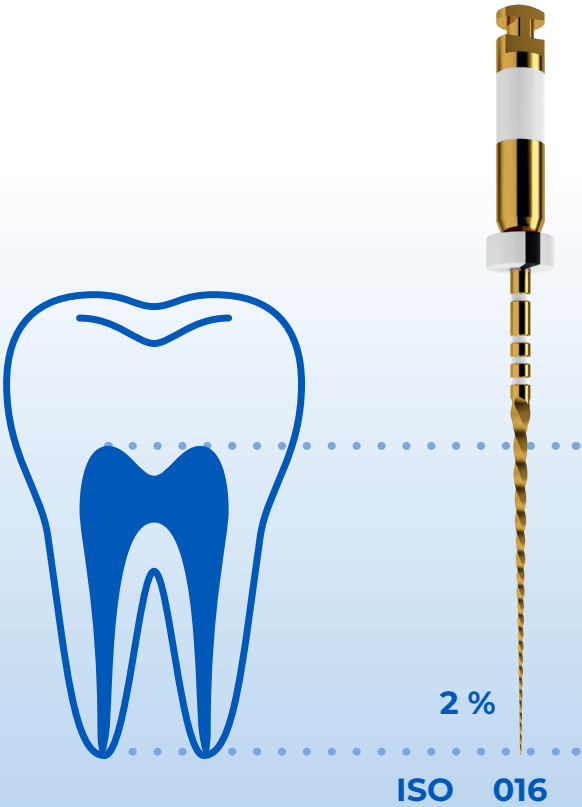

\* The 'satisfied or your money back' guarantee applies only if the following conditions are met: ■ The guarantee is only valid within one hundred days of the invoice date. ■ The guarantee applies to unopened and unused products, with the exception of a box of 6 test files. ■ Products must be returned to the company in their original packaging and over-wrapping and accompanied by the reason for the request for exchange or refund and a photocopy of a quotation or purchase invoice after obtaining a return agreement on the site in the customer's account or from Customer Services. ■ In all other cases, the guarantee cannot be applied.

GO-GLIDER Class IIa medical devices. CFPM Marking CE CFPM On going. Notified body ICIM. **Non-contractual photos.**