


GO-TAPER FLEX protocol (treatment)



After opening the chamber and locating all canals, fill the access cavity with sodium hypochlorite.

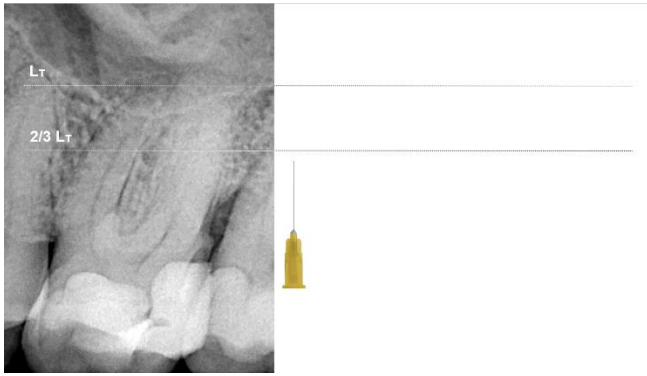


Take a K10 file and insert it passively into the canal, rotating it 1/8th of a turn to the left and right. Move forward without applying pressure and stop when the file stops moving. Note this length.



Take your A1 instrument (purple ring) from the GO-TAPER series and prepare the channel to this length. To do this, insert the instrument in motion into the canal without applying pressure and then remove it brushing the outer wall of the canal. Carry out these pumping movements for 10 seconds, then exit the canal and clean the flute of your instrument. Repeat this action until you have reached the desired length. You have now prepared the coronal 2/3 of the canal.



Irrigate abundantly.

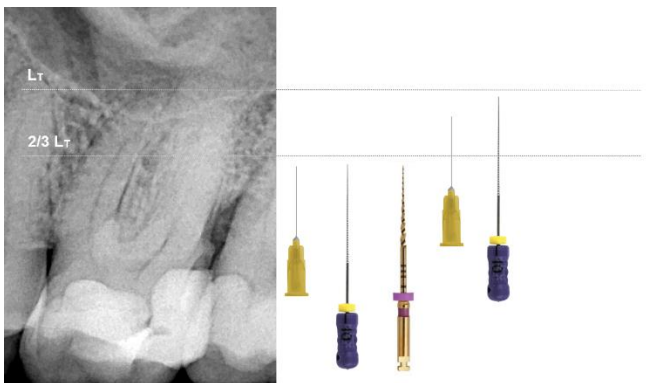

Take again your K10 file and move forward passively like before. In many cases, the file will reach the working length passively. Measure this length using an apex locator. If at this point you cannot reach the working length, do not force it. Remove the K10 file and prepare the canal portion obtained using your A1 instrument, then repeat this step.



Prepare the canal to the working length with your A1 instrument making the same movement as before. Then do the same with your A2 instrument (white ring). Take then the B1 instrument (yellow ring). Bring it to the desired working length without pumping but applying a slight apical pressure. If the instrument does not advance, take it out, clean it and start again. Once the working length attained, do the same using the B2 instrument (red ring). This completes the mechanical preparation of the tooth.